


RESTRICTED

0838
DC/0438/23 dt 07-03-2023

TECHNICAL SPECIFICATION OF SPARES

Ser	Particulars	Description
1.	Name of Item	Cartridge, Hydrosorb Small ✓ (KLEINPATRONE)
2.	Quantity	01(NO)
3.	Part/Patt/Drawing no	123326 (IMC- M.C.4051.00288.0000)
4.	Name of Main Equipment	Analyzer Metal
5.	Equipment Brand	SPECTROMAXx ✓
6.	Equipment Model	✓ LMx07/ LMx06
7.	Equipment Serial no	
8.	Country of Origin (Main Equipment)	Germany
9.	Country of Manufacture	Germany
10.	Year of Manufacture (Spares)	2023 or later
11.	Source of Supply	OEM
12.	Port of Shipment	Any port of Germany
13.	Manufacturer's Name and Address	AIR LIQUIDE, Germany ✓
14.	Supplier/Local Agent	To be mentioned
15.	Certificate and Document of Authentication	Authenticity and Genuineness Certificate
16.	Packing/Labeling	To be packed and labeled for international shipping
17.	Warranty	At least 02 years from date of acceptance
18.	Installation/Compatibility/Interfacing	Item to be installed by supplier
19.	Site visit	The interested bidder may visit the Equipment/ Machine site if it is required

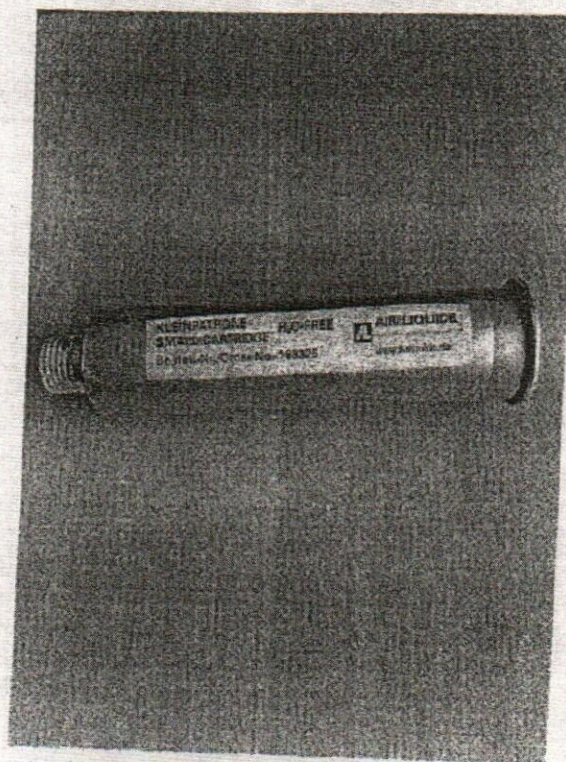

KLEINPATRONE (HYDROSORB CARTIDGE)- H₂O FREE
(For Metal Analyzer- Spectromax)

[Handwritten signature]


NASIM IQBAL
Lt Cdr BN
Officer-in-Charge
BN Dockyard Laboratory

RESTRICTED

114547

TECHNICAL SPECIFICATION OF SPARES

Ser	Particulars	Description
1.	Name of Item	Tube, Molecular Sieve ✓
2.	Quantity	01(NO)
3.	Part/Patt/Drawing no	P4018 (IMC- M.T.1028.00238.0000)
4.	Name of Main Equipment	Argon Gas Purifier (Accessory of Analyzer Metal)
5.	Equipment Brand	SIRCAL
6.	Equipment Model	MP-2000 ✓
7.	Equipment Serial no	
8.	Country of Origin (Main Equipment)	UK
9.	Country of Manufacture	UK
10.	Year of Manufacture (Spares)	2023 or later
11.	Source of Supply	OEM
12.	Port of Shipment	Any port of UK
13.	Manufacturer's Name and Address	Sircal Instruments(UK)Ltd
14.	Supplier/Local Agent	To be mentioned
15.	Certificate and Document of Authentication	Authenticity and Genuineness Certificate
16.	Packing/Labeling	To be packed and labeled for international shipping
17.	Warranty	At least 02 years from date of acceptance
18.	Installation/Compatibility/Interfacing	Item to be installed by supplier/bidder
19.	Site visit	The interested bidder may visit the Equipment/ Machine site if it is required

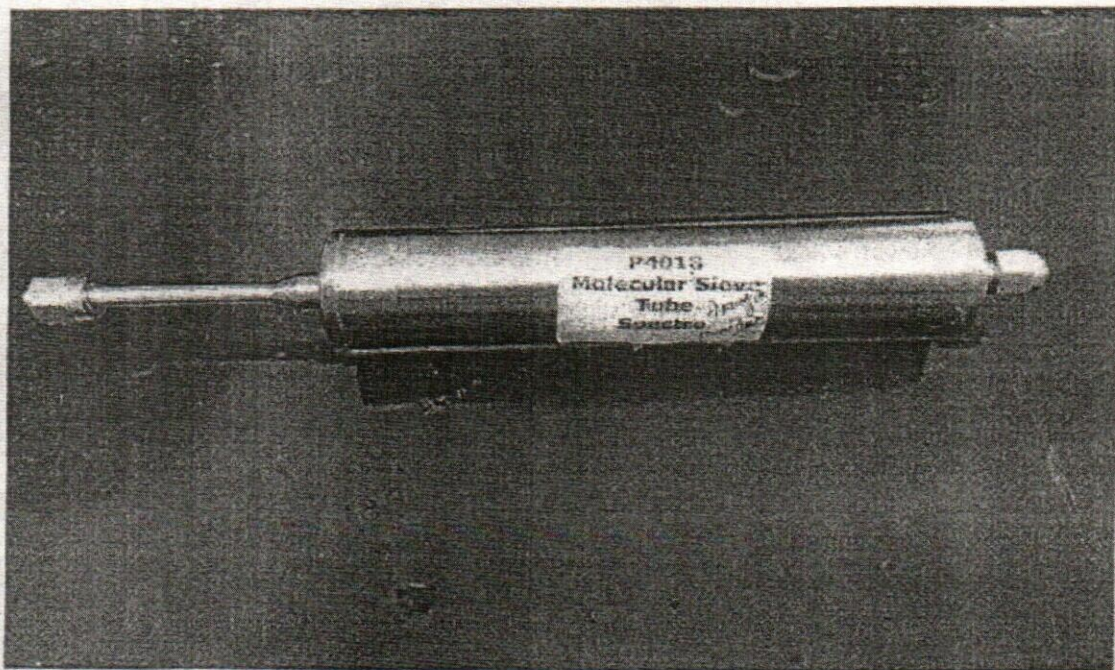

Tube, Molecular Sieve
(For Argon Gas Purifier)

[Signature]

NASIM IQBAL
Lt Cdr BN
Officer-in-Charge
BN Dockyard Laboratory